


Lactic Acid Reflex Change in Ordering and Redraws

Effective Date: April 11th, 2021

Effective April 11th, the following process will occur with all plasma lactic acid orders that are placed in Epic Beaker. There is no change in sample collection tube (**gray-top**).

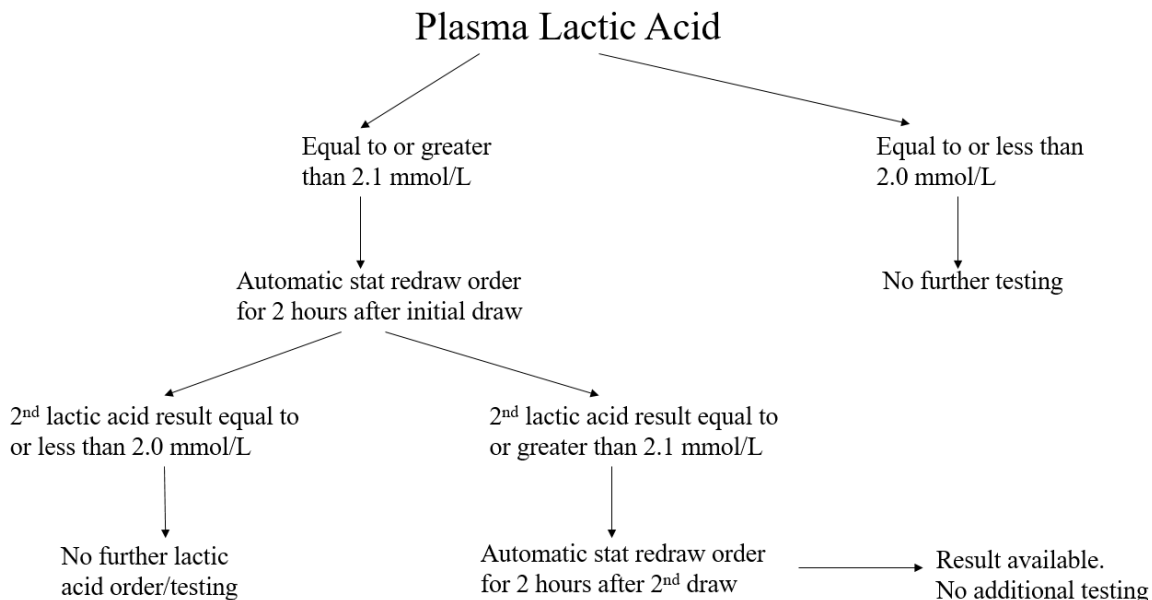

This change has been made at the request of the System Sepsis Committee. The automatic redraw applies only to plasma lactic acid and not to whole blood lactic acid orders. **The new rule will apply to all plasma lactic acid orders for Inpatients and Emergency Center patients.**

It will be included in the following order sets:

- Dearborn, Trenton, Taylor, Wayne, Canton
 - ED Triage protocol possible sepsis [2372]
 - ED adult sepsis/severe sepsis/septic shock [30007]
 - IP adult sepsis/severe sepsis/septic shock [30031]

- Royal Oak, Troy, Farmington Hills, Grosse Pointe
 - ED adult sepsis/severe sepsis/septic shock [3007]
 - IP adult sepsis/severe sepsis/septic shock [3031]

Date submitted: April 5, 2021

Submitted by: Elizabeth Sykes, MD, System Medical Director, Chemistry
Jennifer Pipta, BSN, RN, Beaumont Health Sepsis Coordinator Lead
Zafar Shamoon, MD, Beaumont Health EC Sepsis Physician Lead
Paul Bozyk, MD, Beaumont Health IP Sepsis Physician Lead