

# Beaumont


Pictured below are the approved Nasopharyngeal collection kits for COVID-19 testing.

**NOTE:** Expired products will be accepted (if expiry date is within the last 18 months) due to the national shortage in Covid-19 testing supplies.

Universal Transport Media (VTM, UVT, M4, M5, or M6): Approved for in-house testing and send-outs.



Ruhof VTM (Product Code 354CVTK): Approved for in-house testing only.

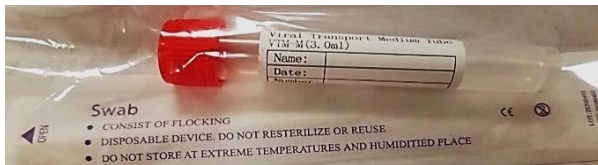

GeneXpert Xpert® Xpert NP Sample Collection Kit



BD ESwab (Green) Collection & Transport System



MedSchenker® Smart Transport Media with provided flocked NP swab




# Beaumont

Pictured below are the approved Nasopharyngeal collection kits for COVID-19 testing.

**NOTE:** Expired products will be accepted (if expiry date is within the last 18 months) due to the national shortage in Covid-19 testing supplies.

Hardy Diagnostics VTM or Copan UTM with provided flocked NP swab

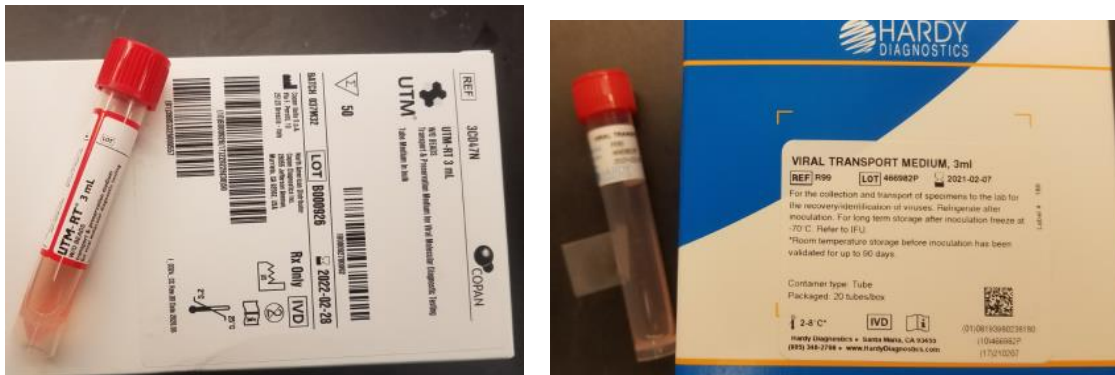

Pictured below are the approved Oropharyngeal collection kits for COVID-19 testing

BD Eswab (White) Collection and Transport System



Starswab® Multitrans System by Starplex Scientific Inc.



Beaumont Laboratory continues to evaluate additional collection devices and will be updating this document accordingly.